

Multichannel Electrochemical Workstation ZIVE MP1 (4CH housing)

*Including Internal FRA
10Volts/1Amp*



*For
Corrosion
Material Testing
Sensor/BioElectrochemistry
Battery/Fuel Cell
Super Capacitor/Solar Cell*

Electrochemical Workstation ZIVE MP1

System Features

- Versatile, high quality multichannel Potentiostat/Galvanostat/Impedance Analyzer
- Standard 4 channel housing system
- Fully independent channels with 14 EIS technique capability including multisine EIS technique at affordable price
- Compact design with Smart LCD per channel
- Current Interrupt IR measurement
IR compensation available(dynamic, positive feedback)
- Wide current ranges(10nA~1A) for various application
(10nA with gain)
- Independent operation by DSP with FPGA per channel
- Built-in FRA in each channel: Impedance measurements
- High speed data sampling time
- 2usec or 3usec depending on data point number
- Fast sweep mode(5000V/sec with 10mV data sampling)
- Internal 542,000 data point storage and test running regardless of PC failure
- Channel expansion is available up to 16 channels via USB hub
- Full software packages are included as standard
 - Corrosion test software package(COR)
 - EIS test software package(EIS)
 - Electrochemical analysis software package(EAS)
 - Energy software package(BAT)
- Voltage pulse or current pulse charge/discharge test(GSM,CDMA etc) and sine wave function for ripple simulation in battery test package & pulse plating available(Bipolar pulse capability)
- Free software upgrade

■ 4 channel housing system



Channel expansion = master + slave option

4ch housing system

1) Example 1

: 6 channel system
= master(4ch) + slave(2ch)

2) Example 2

: 8 channel system
= master(4ch) + slave(4ch)

System

The ZIVE MP1, the outstanding multichannel potentiostat/galvanostat/FRA is the best choice for the complete DC and impedance characterization of corrosion, coatings, sensors and other fundamental electrochemical analysis. And also, its versatile functions make it suited to other application including various energy sources and storage such as fuel cells, batteries, solar cells, and super capacitors.

Each channel is designed under FPGA (Field Programmable Gate Array) and DSP(Digital Signal Processor) control with high speed capability.

- DAC control: Two set of high speed 16bit DAC(50MHz) for offset & scanning
- ADC reading: Two set of 16 bit 500kHz ADC for reading voltage/current and 1 channel 16bit 250kHz ADC for auxiliary data input.
It can provide high frequency EIS, fast pulse techniques and high speed sampling time.

The ZIVE MP1's each channel is equipped with a frequency response analyzer(FRA) and Smart LCD as standard. It also provides high performance impedance measurement over the frequency range 10uHz to 1MHz. The ZRA(zero resistance ammeter) function can measure max. 1Amp in galvanic corrosion technique. The system is supplied with four(4) advanced software packages, which are categorized by application fields. With this advanced software packages, user can widen ZIVE MP1's flexibility.

Versatility

The ZIVE MP1's system comes with one additional analog input(auxiliary voltage input). Each channel can work on same or different experiment at the same time. This model can interface with ZB series external booster for high current applications. The channels are expandable by adding slave channels up to 16 channels.

Safety

- When communication failure occurs between a PC and ZIVE MP1, the running channels will continue experiments and, at the same time, save the data into ZIVE memory up to 542,000 data point set. When the communication is recovered, ZIVE MP1 will transfer saved data to the PC. User can transfer data set from ZIVE MP1 to PC at any time. This function is highly efficient for long-term experiment and protects experiments from unexpected PC failure.
- Users can define safety condition setting by inputting his/her own safety levels for voltage, and current etc. If the measurement value exceeds the setting value, the system will automatically stop to protect the system and cell.
- If the control value of voltage or current is different from the measured value, the experiment will stop automatically to protect the cell.
- Automatic calibration function is supplied for user calibration.


Maintenance

- The system has its own hardware parameters and calibration data.
- Each channel is plug & play type and easy to install or to be removed.

Application

The ZIVE MP1 multichannel electrochemical workstation is ideal for fundamental research in electrochemistry, development and quality assurance of new sensors, corrosion/coatings, electrode material, membrane, conducting polymer, evaluation power device research such as battery materials, fuel cells, super capacitors and solar cells.

■ General Electrochemistry



The ZIVE MP1 is also suitable for the development of bio-research, electron transfer kinetic studies and electrochemical analysis of compounds at low trace levels, where multichannel DC and impedance analysis is beneficial in providing high throughput of results.

Electrochemical Workstation ZIVE MP1

Corrosion



The system is suitable for measuring low corrosion rates and EIS test to evaluate corrosion. ZRA function is supplied for galvanic corrosion measurement.

Sensors



The ZIVE MP1 can be used for sensor research using with DNA chips or screen printed electrodes. System's minimum current range is 10nA(with gain) with EIS capability.

Batteries



The system is very well adapted for researches on the cycling behavior of battery. It supports EVS (electrochemical voltage spectroscopy)/GITT/PITT test. Fast pulse capability for GSM, CDMA test is included in battery test software package. Pulse profile measurement function to check pulse shape is available. For ripple simulation test, sine wave charging/discharging is available.

Fuel Cells



The ZIVE MP1 is ideal for characterizing the fuel cells and anodic/cathodic process mechanism at development and research grade. This system can be directly used for PEMFC, DMFC, and DEFC etc. Automatic current ranging potentiostatic/galvanostatic IV curve is available.

Super Capacitors



The ZIVE MP1 has fast potentiostat circuit with high speed data acquisition. This function is well applicable to super capacitor testing. Charging/discharging capability is used for this application.

Solar Cells




Solar cell development and production requires extensive material and device testing to improve efficiency and match individual cells for panel construction.

Main Software SM

The Smart Manager (SM) is to control ZIVE MP1 model and it provides user defined sequential test by using sequence file, technique menu and batch file. The batch file allows the users to do a serial test by combining sequence files and/or technique files.

The SM software is easy to use and supports various electrochemical experiments including functions of system control, schedule file editor, real time graph, analysis graph, user calibration, and data file treatment etc.

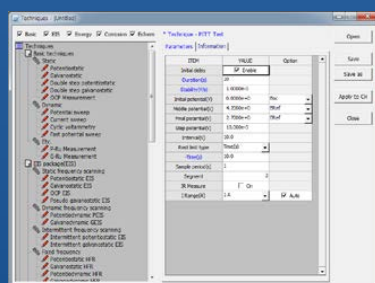


Technique list

Basic Techniques

Basic techniques with standard functions


- 1) Potentiostatic
- 2) Galvanostatic
- 3) Double step potentiostatic
- 4) Double step galvanostatic
- 5) OCP measurement
- 6) Potential sweep
- 7) Current sweep
- 8) Cyclic voltammetry
- 9) Fast potential sweep
- 10) Potentiostatic Ru measurement
- 11) Galvanostatic Ru measurement

The above functions can be used sequentially by step control function.

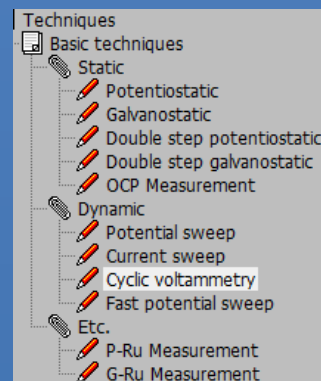

Sequence editor

User can design his/her experiment procedure by using TASK sequential routine editor.

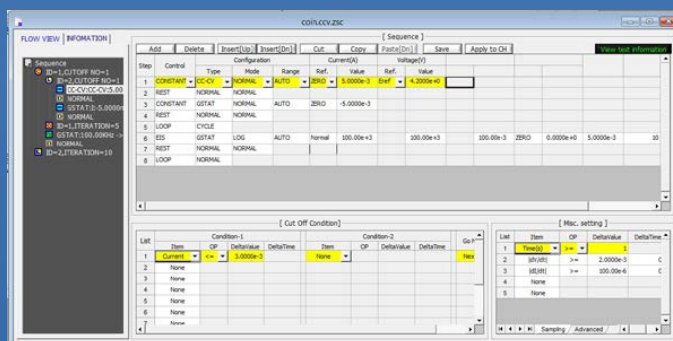

Sequence editor

Control Task Parameters

| Control Mode | | |
|--------------|------------------------------|---|
| constant | GSTAT | constant current control |
| | Crate | constant Crate control |
| | PSTAT | constant voltage control |
| | POWER | constant power control |
| | LOAD | constant load control |
| | CC-CV | constant current constant voltage control |
| | Crate-CV | Crate constant voltage control |
| | CP-CV | constant power constant voltage control |
| | CL-CV | constant load constant voltage control |
| | Id | Id control |
| | Is | Is control |
| | OCP | OCP control |
| | Step | GSTAT |
| PSTAT | | potential step control |
| Sweep | GSTAT | current sweep control |
| | FAST-G | fast current sweep control |
| | PSTAT | potential sweep control |
| | FAST-P | fast potential sweep control |
| EIS | GSTAT | galvanostatic EIS |
| | PSTAT | potentiostatic EIS |
| | OCP | OCP EIS |
| | PSUEDO | pseudo galvanostatic EIS |
| | HFR G | galvanostatic HFR |
| | HFR P | potentiostatic HFR |
| | MsineG | galvanostatic multisine EIS |
| MsineP | potentiostatic multisine EIS | |
| Rest | | rest control |
| ZRA | | ZRA control |
| Loop | | loop control |
| Pulse | Vpulse | voltage pulse control |
| | Ipulse | current pulse control |
| | GSINE | current sine wave control |
| | PSINE | potential sine wave control |
| | | |

Electrochemical Workstation ZIVE MP1

- Constant potential, current, C-rate, power, load, OCP
- Sweep potential, current
- Fast sweep potential, current
- Staircase potential, current
- CC-CV, CP-CV, CL-CV, Crate-CV control
- Id, Is control
- EIS control
- Pulse or sinewave control
- Rest(voltage monitoring only)
- Loop(cycle) control

| Item | OP | DeltaValue |
|------------|----|------------|
| Step Time | >= | 30 |
| None | | |
| Step End | | |
| Step Time | | |
| Current | | |
| I Density | | |
| Voltage | | |
| [Capacity] | | |
| -dV | | |
| dI/dt | | |
| dV/dt | | |
| dT/dt | | |
| Temp.(C) | | |
| AUX1 | | |
| AUX2 | | |
| AUX3 | | |
| Test Time | | |
| Loop Time | | |
| Cycle Time | | |
| Eoc | | |
| [Whr] | | |
| LCC(%) | | |
| LCD(%) | | |
| FCC(%) | | |
| FCD(%) | | |
| Power(W) | | |
| SumQ(Ah) | | |
| SumE(Whr) | | |
| Loop Next | | |
| DI Ch. | | |
| Crate | | |

Cutoff Condition

- Cut-off(Vertex) Condition
 - Time(step, test, loop, cycle)
 - Current, current density
 - Voltage
 - Capacity
 - C-rate
 - -dV
 - |dV/dt|
 - |dI/dt|
 - Aux1
 - Eoc
 - etc.
- Sampling Condition
 - Time, |dI/dt|, |dV/dt|, |dA1/dt|, burst time

Flow View

- User can see the sequence flow at a glance.

| Step | Cont |
|------|--------|
| 1 | CONSTA |
| 2 | CONSTA |
| 3 | CONSTA |
| 4 | REST |
| 5 | LOOP |
| 6 | EIS |
| 7 | REST |
| 8 | LOOP |

Flow view

Batch function


User can design batch file including multiple technique files and/or sequence files. With this batch file, user can experiment several techniques/sequence in series automatically.

Smart Manager Advanced Software Packages


For a wide range of application, advanced software packages for specific experimental techniques are available.

EIS Software Package(EISe)


1. Potentiostatic EIS
2. Galvanostatic EIS
3. Pseudo galvanostatic EIS
4. OCP^(*) EIS
5. Potentiodynamic PEIS
6. Galvanodynamic GEIS
7. Potentiodynamic HFR
8. Galvanodynamic HFR
9. Potentiostatic HFR monitor
10. Galvanostatic HFR monitor
11. Multisine potentiostatic EIS
12. Multisine galvanostatic EIS
13. Intermittent potentiostatic EIS
14. Intermittent galvanostatic EIS

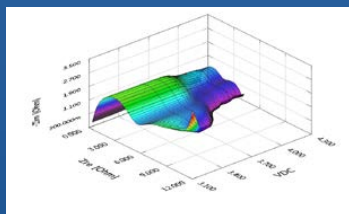


Coin Cell Intermittent PEIS
3D Nyquist Plot By ZMAN



OCP EIS



Potentiodynamic PEIS



Rs, Cp & Idc vs Vdc plot

Energy Software Package(BATe)


BATe software supports IR measurement.

1. Battery test techniques


- CC/CV test for cycle life test of lithium battery
- CC/CC test for cycle life test of NiCd or NiMH battery
- Discharging test
- EVS(Electrochemical voltage spectroscopy)
- Variable scan rate CV
- Potentiostatic IV curve
- Galvanostatic IV curve
- Steadystate CV
- GITT
- PITT



CC/CV test



CC/CC test




EVS test



Variable scan rate CV



Pulse shape profile monitor(micro seconds order)



Current sine wave(charge ripple simulation)

2. Control mode

- Charge: CC, CC-CV, pulse, sine wave
- Discharge: CC, CP, CR, pulse, sine wave

3. Cutoff condition


- Time, voltage, current, power, AuxV, etc.

Various battery charge/discharge test is available including pulse discharge or GSM and CDMA application.

(*1) The system measures open circuit potential before each frequency change and applies AC sine wave on this potential.

■ Electrochemical Analysis Software Package(EASE)

- Step techniques
 - CA(Chronoamperometry)
 - CC(Chronocoulometry)
 - CP(Chronopotentiometry)
- Sweep techniques
 - LSV(Linear sweep voltammetry)
 - SDV(Sampled DC voltammetry)
 - Fast CV
 - Fast LSV
- Pulsed techniques
 - DPV(Differential pulse voltammetry)
 - SWV(Square wave voltammetry)
 - DPA(Diff. pulse amperometry)
 - NPV(Normal pulsed voltammetry)
 - RNPV(Reverse normal pulse voltammetry)
 - DNPV(Differential normal pulse voltammetry)

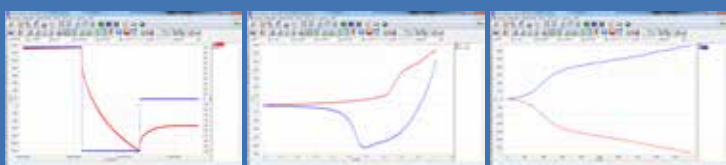


50usec sampling Sampled DC voltammetry NPV & RNPV overlay


■ Corrosion Software Package(CORE)

Corrosion technique supports IR compensation.

1. Tafel(Tafel experiment)
2. Rp(Polarization resistance)
3. Potentiodynamic
4. Galvanodynamic
5. Cyclic polarization
6. Ecorr vs. time
7. Galvanic corrosion
8. RpEc trend
9. Reactivation potential
10. Critical pitting potential
11. Potentiostatic ECN
12. Galvanostatic ECN
13. ZRA mode ECN

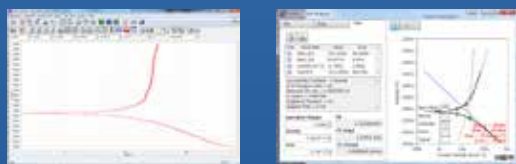

Tafel experiment

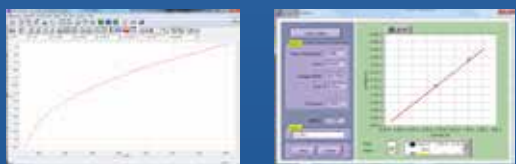

Rp
(Polarization resistance)



CYPOL(Cyclic polarization resistance)

Control & Real Time Graph

Smart Manager provides 2 kinds of control & data acquisition with real time graph.




Multichannel control panel Multichannel data monitor (EIS data/DC data selectable) Multichannel real time graph

User can control and monitor for specific channel in details and he/she can monitor data in VOI(value of interest) window and channel status in one window. Real time graph's X Y axis format will be changed per technique automatically. It can be also defined by user's demand per techniques.




For experiment using sequence file or batch file, user can designate X,Y parameter on three different real time graphs. This graph shows the changes and can monitor and control the channel at the same time.

Real time graph and VOI will be changed depending on DC test or impedance test automatically. Virtual control panel always displays the graph for recent test result. For impedance measurement, wave monitor will be displayed on real time graph to check wave's quality. This monitor can be switched to Lissajous (I vs. E) plot.



■ Strip Chart



Strip chart recorder function provides real graph function independently. You can monitor 2 Y axis data such as voltage, current, auxV, power, and capacity etc. in real time. You can also select channels that need to be monitored and can set maximum data point for strip chart length.


■ Simple Monitor



This display window is for monitoring the major data values and channel status for multiple channel operation.

| Simple monitor | | | |
|--|---|---|--|
| CH01 RUNNING TIME: 0:01:07 VOLT: 111.7323mV CURR: 27.2525uA CAPA: 1.9743uF | CH02 RUNNING TIME: 0:04:17 FRQ: 177.8300kHz RNG: 3.1681MHz FREQ: 175.7812kHz | CH03 READY TIME: 0:01:03 VOLT: -1.2207mV CURR: 0.000 A CAPA: 0.000 uF | CH04 READY TIME: 0:01:59 VOLT: -216.527mV CURR: 0.000 A CAPA: 0.360 uF |
| CH05 READY TIME: 0:01:54 VOLT: 244.2022mV CURR: 0.000 A CAPA: 0.000 uF | CH06 RUNNING TIME: 0:00:48 VOLT: 192.7267mV CURR: 11.1287uA CAPA: 820.2281 uF | CH07 READY TIME: 0:01:58 VOLT: -410.3516mV CURR: 0.000 A CAPA: 0.000 uF | CH08 READY TIME: 0:01:58 VOLT: -245.527mV CURR: 0.000 A CAPA: 0.360 uF |

■ Graph

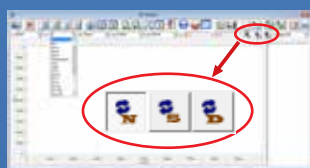Smart Manager's graph function is to simplify the operation. There are 3 kinds of graph per experiment. You can change X, Y1, Y2, Y3, Y4 axis parameter as you want. Each graph provides shortcut buttons. When you click these buttons, the graph format will be changed accordingly.




In DC and Cycle graph, whenever you click  or , the parameters which are related to current such as current, capacity, energy, power, load, etc., are changed into calculated specific value or density value, respectively.

 : value divided by weight

 : value divided by active area

1. DC graph

For general data display

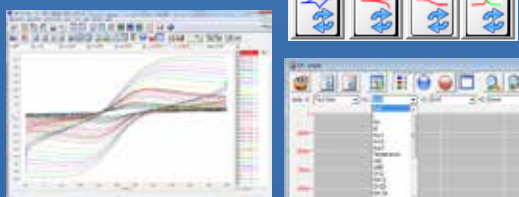

4 Shortcut buttons:

I vs. V, E vs. LogI, V, I vs. time, V vs. Q.

Graph parameters: Time, Eref, I, Eoc, Id, AuxV, LogI, Load, ChQ, DchQ, ChQs, DchQs, Ch P, Dch P, Ch-Wh, Dch-Wh, Sum Wh, Sum Q, Sum |Q|, |Q|, Rp, dQ/dV

2. EIS graph


For EIS data display



3 Shortcut buttons

Nyquist plot, Bode plot, Cs vs. frequency.

Graph parameters: Frequency, Zre, -Zim, Zmag, Zph, Y, Yimg, Y, |Y|, Yph, LogZ, LogY, Rs(R-C), Cs(R-C), Rp(R|C), Cp(R|C), Rs(R-L), Ls(R-L), Q(R-L), time, Vdc, Idc, Aux(1)



3D Bode Plot by ZMAN
Technique used: Potentiodynamic Impedance Measurement by using a corrosion cell

3. BAT graph


For battery cycle data display



3 Shortcut buttons:

cycle capacity, cycle average, Log(cycle No) vs. depth of discharge plot.
Graph parameters: cycle number, Ch Q, Dch Q, Sum Q, Coulomb Eff, Ch-Wh, Dch-Wh, Sum Wh, Energy Eff, MinV, MaxV, ChQs, DchQ, ChVavg, DchVavg, Vavg

■ Data Export to ASCII & Excel File

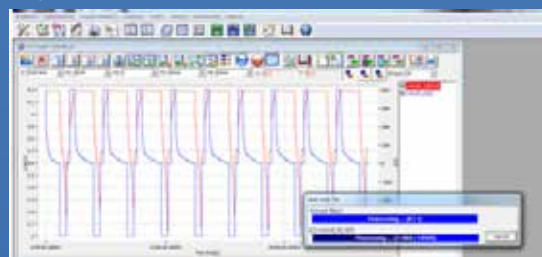

Selectable between 'Convert data on graph only' and 'Convert selected file(s)'

Data Analysis Software


ZIVE data file can be used for analysis by using external IVMAN™ software for DC analysis, IVMAN DA™ software for battery data analysis, IVMAN PA™ software for photo-voltaic cell data analysis and ZMAN™ software for EIS data analysis without license.

ZMAN™ EIS Data Analysis Software


- Model simulation and fitting
- 2D- and 3D-Bode- and Nyquist plots
- Automatic equivalent circuit model search function
- Project concept to handle multiple EIS data analysis
- Parameter plot from fitted elements value
- Compatible with data format from Zahner, Gamry, Ametek etc. (License code is needed.)
- Various weighting algorithm
- Model library and user model
- KK plot
- Batch fitting for project data
- Impedance parameter simulation
- Interpolate bad data
- Black-Nichols plot
- 3D graph setting option
- Improved model editor
- Application model library for automatic searching
- Parameter simulation of model
- Genetic algorithm option for initial guessing
- Automatic initial guessing
- Trace movie function on fitting
- Free for ZIVE's data format (*.seo, *.wis) analysis (No license code required.)
- Circle fitting
- Data editing available (insert, delete, edit)
- Add/subtract element parameters
- Add/subtract model parameters
- Impedance, Z in polar, admittance, Y in Polar, modulus, M in polar, dielectric constant, E in polar. data display

Electrochemical Workstation ZIVE MP1



- Empty cell capacitance calculation
- Find file function
- Data replacement by formula function
- Cursor data display
- Model finding result automatic sorting by Chi square value
- R, C R, L R, Q preview & graphic
- ZHIT function
- Mott-Schottky analysis
- Donor density vs. Vfb graph
- C vs. voltage graph




Parameter simulation




Element add/subtraction

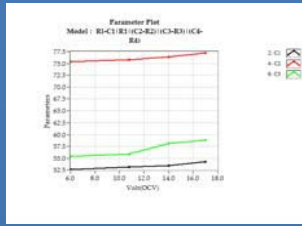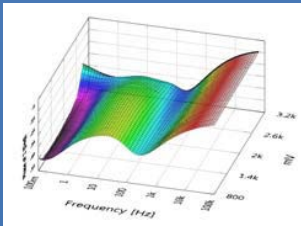


3D Bode plot for series measurement Parameter plot



Importing 3rd parties ASCII data file




Project manager with data preview




Cursor data display




Data replacement by formula function




Fitting display




Model editor & model library




Automatic model searching




LEVM fitting




Finding data file menu




Circular fitting




2D Nyquist plot




2D Bode plot




Rp,Cp vs frequency (R/C)




Empty cell capacitance




Donor density vs. Vfb graph and analysis




KK consistency



Mott-Schottky analysis window

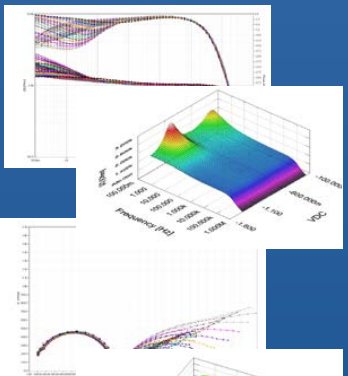

Bode & Nyquist overlay & 3D plots



C/R-V graph

IVMAN™ DC Data Analysis Software



- IVMAN™ software package consists of
 - IVMAN software
 - IVMAN utilities
 - IVMAN differential analysis software
 - IVMAN photo voltaic cell analysis.
 - IVMAN Tafel analysis
 - IVMAN extractor
 - IVMAN peak find module




IVMAN DA™ Battery Test Data Analysis Software

- Battery test data analysis
- Electrochemical voltage spectroscopy (dQ/dV vs. V)
- Voltage vs. Capacity analysis (V vs. Q)
- Cycle graph (Q vs. cycle)
- Differential voltage graph(dV/dQ vs. Q)




Measured data

V vs. Q

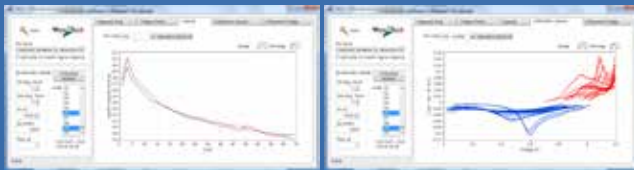

Cycle graph

dQ/dV vs. V

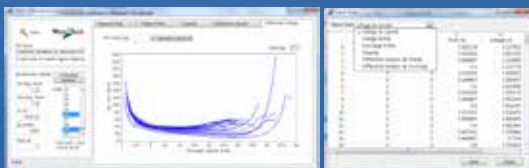


dV/dQ vs. Q

Export ASCII file



IVMAN™ Photovoltaic Cell Analysis

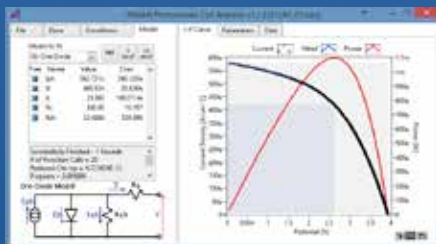


- Automatic analysis of parameters
 - : open circuit voltage, open circuit current, max. power, efficiency
 - photo induced current, diode quality factor, series resistance, etc.




IVMAN™ Main Software

- Ideal for DC corrosion data analysis and electro-analytical data analysis
- Initial guessing function on Tafel analysis
- Polarization resistance fitting
- 3D graph
- Find peak function
- Interpolation, differentiation, integration etc.
- Reporting function

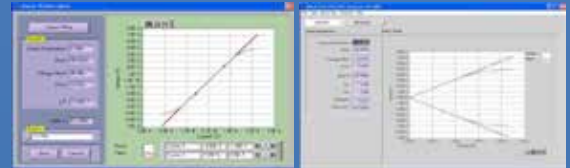

Polarization resistance fitting

Polarization analysis result

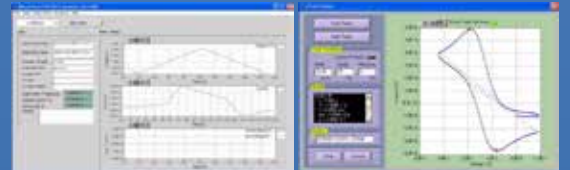

Time graph

Find peak menu



CV graph

3D graph




Edit data menu

Universal graph



IVMAN TA™ Tafel Analysis


- Simple Tafel calculation

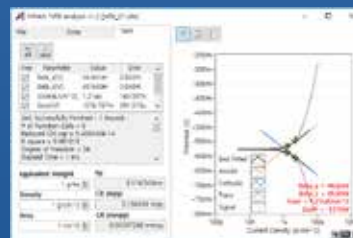


Electrochemical Workstation ZIVE MP1

IVMAN EX™ Extractor

- Extracting data by cycle number or step
- Exporting ASCII file

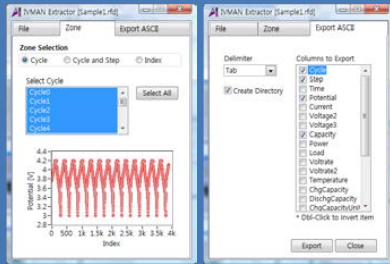


- Pouch Cell Jig
 - contact type
 - a) pull-down contact type with adjustable contact probe's width
 - b) banana connector for cell cable connection
 - 4 contact point type (Kelvin probe)

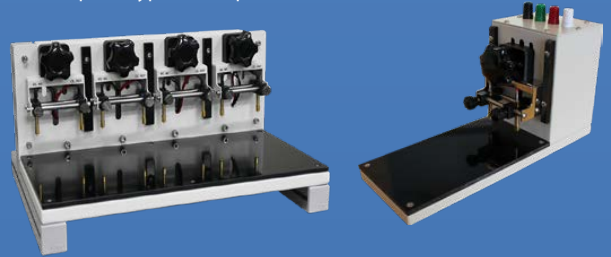

IVMAN PF™ Peak Find Module

- Independent peak finding software

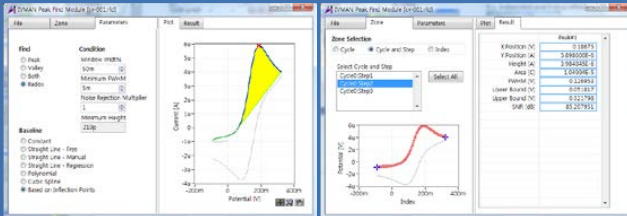

- Coin Cell Holder
 - D-SUB connector type



Optional Accessories

- Power Booster
 - for high voltage/high current application
 - modular type design
 - EIS capability
 - sine wave simulation available



- Redox Flow Battery Test System
 - for charge/discharge test of a single cell
 - impedance measurement available
 - temperature control and measurement
 - electrolyte flow control with a dual channel peristaltic pump
 - max. 4 channel control with a PC
 - support various safety functions
 - system configuration :
ZIVE SP5 Electrochemical workstation + RFC1 flow cell controller



- Battery Jig & Coin Cell Jig
 - for cylindrical cell or coin cell
 - 4 or 2 contact pin depending on models
 - rack type is available.




- Flow Cell Controller
 - MFCs and/or liquid pumps control
 - heating and cooling control
 - valve control
(gas flowing on/off, dry/wet gas selection etc.)
 - rotator control
 - pressure regulator control
 - measurement of temperature, voltage, pressure, humidity etc.



Electrochemical Workstation ZIVE MP1

- Black Box
- for photoelectrochemical experiments



- Cell Kit



Corrosion Cell Kit



Flat Cell Kit

- Single Cell Hardware Fixture
- for PEMFC and DMFC
- max. temp.: 120°C or 180°C
- active area :
5, 9, 25, 50, 100cm²
- MEA is not included.





Plate Test Cell



Plate Test Cell

- Membrane Conductivity Cell
- for 5, 9 and 25cm² fuel cell hardware fixture
- material : PEEK(cell body), platinum(wire)
- operating temp. : up to 130°C



Photoelectrochemical Cell



Permeation Cell

- Through-Plane Conductivity Test Jig
- for through plane conductivity measurement
- 2 probe type



- Flat Specimen Holder



- Pt Plate Counter Electrode



- Universal Electrode Holder
- electrode and glass vial are not included.



- Faraday Cage
- size : 300 x 300 x 398mm(WxDxH)



Specification

| Main System | |
|---------------------------|--|
| PC communication | USB2.0 high speed |
| Line voltage | 100~240VAC, 50/60Hz, 1Amp |
| Max. channel no. per unit | 4 channels per unit (4ch housing system) |
| Channel expansion | 16 channel expandable per PC |
| Max. output power | 12Watt per channel |
| Size 4 channel housing | 199x455x388mm (WxDxH) |

| System | |
|----------------------|---|
| Cell cable | 1 meter shielded type(standard) working, reference, counter, working sense, Auxiliary V |
| Control DAC | DSP with FPGA 2x16bit DAC(50MHz) for bias & scan |
| Data acquisition ADC | 2x16bit ADCs(500kHz) for voltage, current 1x16bit ADCs(250kHz) for auxiliary reading |
| Calibration | Automatic |
| Filter selection | 4ea(5Hz, 1kHz, 500kHz, 5MHz) |
| Scan rate | 0~200V/sec in common mode 0~5000V/sec in fast mode |
| Front panel LED | Busy, Run |
| Internal data memory | 542,000 points |

| Power Amplifier(CE) | |
|-------------------------|-----------------|
| Power | 12Watt (12V@1A) |
| Compliance voltage | ±12V |
| Max. current | ±1A |
| Control speed selection | 4ea |
| Bandwidth | 2MHz |
| Slew rate | 10V/usec |

| Potentiostat Mode (voltage control) | |
|-------------------------------------|--|
| Voltage control | |
| Control voltage range | ±10V, ±1V, ±100mV |
| Voltage resolution | 16 bit per each range |
| Voltage accuracy | ±1mV ±0.05% of setting(gain x1) |
| Max. scan range | ±10V vs. ref. E |
| Current measurement | |
| Current range | 9 ranges(auto/manual setting) 100nA ~ 1A 10nA with gain |
| Current resolution | 16 bit 30uA, 3uA, 300nA, 30nA, 3nA, 300pA, 30pA, 3pA (300fA with gain) |
| Current accuracy | ±10pA ±0.1% f.s.(gain x1) > 100nA |

| Galvanostat Mode (current control) | |
|------------------------------------|--|
| Current control | |
| Control current range | max. ±1A ± full scale depending on selected range |
| Current resolution | 16 bit 30uA, 3uA, 300nA, 30nA, 3nA, 300pA, 30pA, 3pA (300fA with gain) |
| Current accuracy | ±10pA ±0.1% f.s.(gain x1) > 100nA f.s. |
| Voltage measurement | |
| Voltage range | 10V, 1V, 100mV |
| Voltage resolution | 16 bit 0.3mV, 30uV, 3uV |
| Voltage accuracy | ±1mV ±0.05% of reading(gain x1) |

| Electrometer | |
|--------------------|-----------------------------|
| Max. input voltage | ±10V |
| Input impedance | 2x10 ¹³ Ω 4.5pF |
| Bandwidth | >22MHz |
| CMRR | >114dB |

| EIS(Internal FRA) for System | |
|------------------------------|---|
| Frequency range | 10uHz~1MHz |
| Frequency accuracy | 0.01% |
| Frequency resolution | 5000/decade |
| Amplitude | 0.1mV~5Vrms (Potentiostatic) 0.1~70% f.s. (Galvanostatic) |
| Mode | Static EIS: Potentiostatic, Galvanostatic, Pseudogalvanostatic, OCP Dynamic EIS: Potentiodynamic, Galvanodynamic Fixed frequency impedance: Potentiostatic, Galvanostatic, Potentiodynamic, Galvanodynamic Multisine EIS: Potentiostatic, Galvanostatic Intermittent PEIS/GEIS |

| Interfaces for System | |
|----------------------------|---------------------------|
| Auxiliary port | |
| Auxiliary voltage input | 1 analog input: ±10V |
| Zero resistance ammeter | 100nA~1A ranges |
| External booster interface | Via booster I/F cable |
| Sync terminal | For channel synchronizing |

| Smart LCD Display per channel | |
|-------------------------------|---|
| DC mode | Control value, E value, I value E range, I range |
| EIS mode | Frequency, Magnitude, Phase E range, I range |
| Operation status | Mode: PST, GST, ZRA, EIS, CC, CV, CP, CR Status: Cell On, Run, Error |

| Software | |
|--------------------------|---|
| Max. step per experiment | 1000 |
| Shutdown safety limits | Voltage, current, power, AuxV etc. |
| Max. sampling rate | 2usec or 3usec depending on data point number |
| Min. sampling time | Unlimited |
| Sampling condition | Time, dv/dt, dl/dt, etc. |

| PC Requirement | |
|------------------|--------------------------------|
| Operating system | Windows 7/8/10(32bit/64bit OS) |
| PC specification | Pentium4, RAM 1GB or higher |
| Display | 1600x900 high color or higher |
| USB | High speed 2.0 |

| General | |
|------------------------|----------------------------------|
| Dummy cell | One external dummy cell included |
| Impedance analysis S/W | ZMAN™ software |
| DC data analysis S/W | IVMAN™ software package |

The specifications are subject to change without notice.
Windows is a registered trade mark of Microsoft Corporation.

Designed by

ZIVE LAB
www.zivelab.com

WonATech

WonATech Co., Ltd.
7, Neunganmal 1-gil, Seocho-gu,
Seoul, 06801, Korea
Phone: +82-2-578-6516
Fax: +82-2-576-2635
e-mail) sales@wonatech.com
website: www.wonatech.com

Local Distributor



ISO 9000 & ISO 14000 Qualified



CE Certified